

Minutes of Pre-Bid Conference held Pre-bid Conference  
held on 12.09.2019 at 11.00 a.m . at CSIR - IHBT, Palampur, HP

Purchase of Continuous Centrifuge  
against Tender No. 4/5 ( 319) - Pur dated 23/08/2019

The following attended the conference.

**From Technical & Purchase Committee ( T&PC)**


Dr.Vipin Hallan,	Senior Principal Scientist	Chairman
Dr Y.Padwad	Sr Scientist	Member
Dr S.Bhushan	Principal Scientist	Member
Dr.Dharam Singh	Senior Scientist	IO-Member
Shri.Amarjeet	SO (G)	Member
Shri S.N.Gulia	FAO	Member
Shri S.Gnanaprakasam	COSP	Member - Convenor


**From Bidders:**

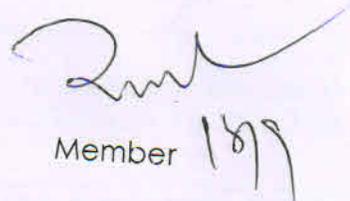
1. M/s. Alfa Laval India Private Limited, New Delhi


Represented by Shri.Sujeet  
Tiwari, Area Sales Manager


The TPC had clarifications given for the issues raised by the above firm during pre-bid conference and had given other modifications / additions to the tender document and are given in Annexure A.


  
Member  
15/9/2019

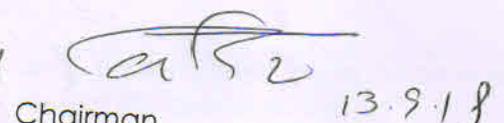
  
Member  
13/9/19

  
Member  
18/9

  
Member (IO)  
13/09/19

  
FAO  
13.9.19

  
COSP  
13/9/19

  
Chairman  
13.9.19

S.N	Query	CSIR - IHBTI's reply
1	Specification 4.2.2 - Details of Electropolishing	Vessel finish internal all wetted parts: mechanical/electro-polish Ra ≤ 0.8 μm.
2	Specification 6 Whether only CIP pump is required	System should be designed to support automatic CIP Process and compatible CIP Pump to be provided along with system
3	Specification 10 cGMP certificate required.	Following documents for cGMP validation should be provided by the successful vendor along with the system  a. Documents for design qualification ( DQ) b. Documents for installation qualification ( IQ) c. Documents for operational qualification ( OQ)
4	Acceptance certificate to be issued within 30 days from the date of receipt of equipment at site	Acceptance certificate will be issued once installation and commissioning is completed. Installation and commissioning is to be completed within 30 days from the date of receipt of equipment at site.
5	Balance payment 20% will be released on acceptance	Balance 20% payment will be released as per SCC Clause 9 – GCC 2.22.1
6	The maximum amount to penalty shall be 5% for 10 weeks	The maximum amount to penalty shall be as per SCC Clause 10 GCC 2.27.1
<b>ADDITIONS to tender conditions</b>	1. Delivery period	The supply shall be completed within 4 months from the date of PO
	2. Installation	Installation shall be completed within 1 month from the date of receipt of material at site.

f. haram  
13/9/19

2421  
13/9/19

2421  
13.9.19

3p  
13/09/2019

2421  
13.9.19

